


QUANTIFICATION REPORT

Experiment Information:

Assay Type	HBV DNA Absolute Quantification
Instrument S/N	Bio-Rad CFX96™ REAL-TIME System
Run Date	10/23/2023 15:12PM

QUANTIFICATION DATA FOR SAMPLE: SURENDER-39481

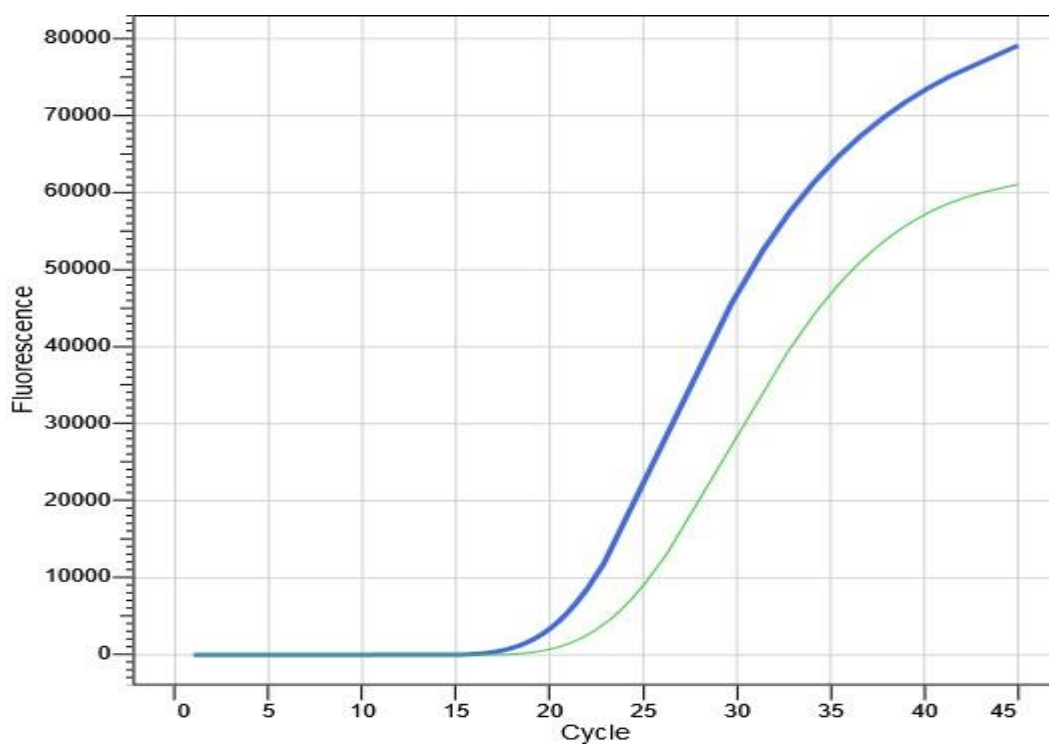

S. No.	Colour	Name	Type	Ct	Given Conc. (copies)	Calc. Conc.
1	■	SURENDER-39481	HBV	20.55	NA	43800000.7 IU/mL
2	■	SURENDER-39481	IPC	24.11	NA	NA