


QUANTIFICATION REPORT

Experiment Information:

Assay Type	HLA B-27 Absolute Quantification
User	IMMUNO DIAGNOSTICS PVT. LTD.
Instrument S/N	Bio-Rad CFX96™ REAL-TIME System
Run Date	4/15/2024

QUANTIFICATION DATA FOR SAMPLE: SARITA-27817

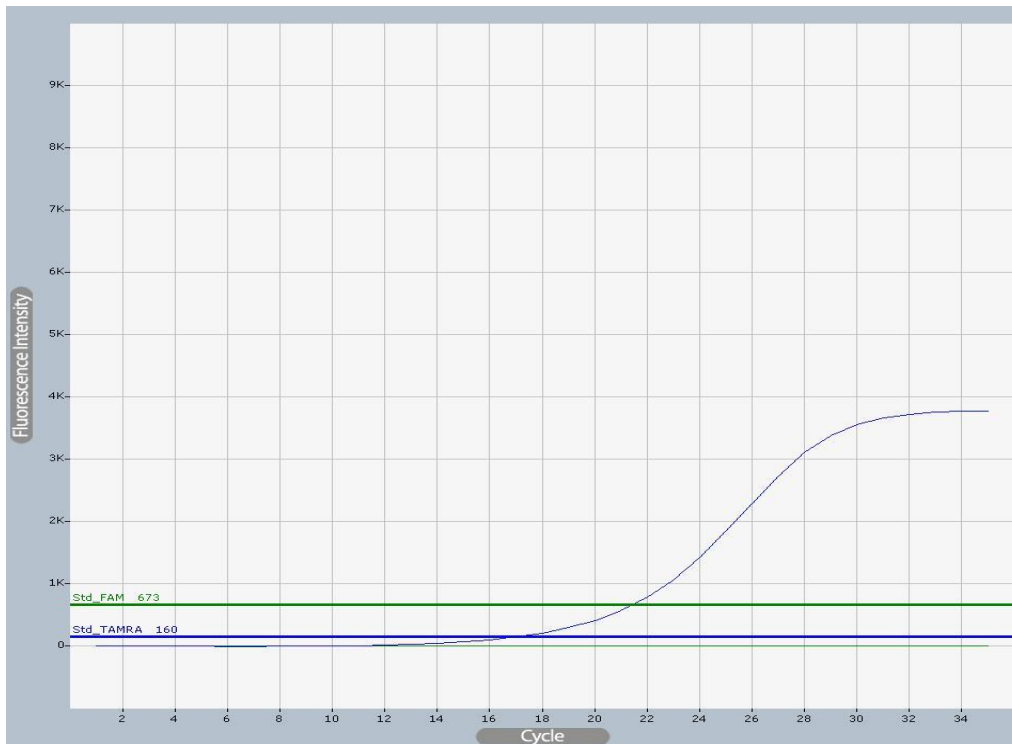

SNo	Colour	Name	Type	Ct	Given Conc (copies)	Calc Conc (copies)
1	■	SARITA-27817	HLA B-27	Undetermined	NA	NA
2	■	SARITA-27817	IPC	16.75	NA	NA