


QUANTIFICATION REPORT

Experiment Information:

Assay Type	HLA B-27 Absolute Quantification
User	IMMUNO DIAGNOSTICS PVT. LTD.
Instrument S/N	Bio-Rad CFX96™ REAL-TIME System
Run Date	5/6/2024

QUANTIFICATION DATA FOR SAMPLE :ATINDER 10208002-6230

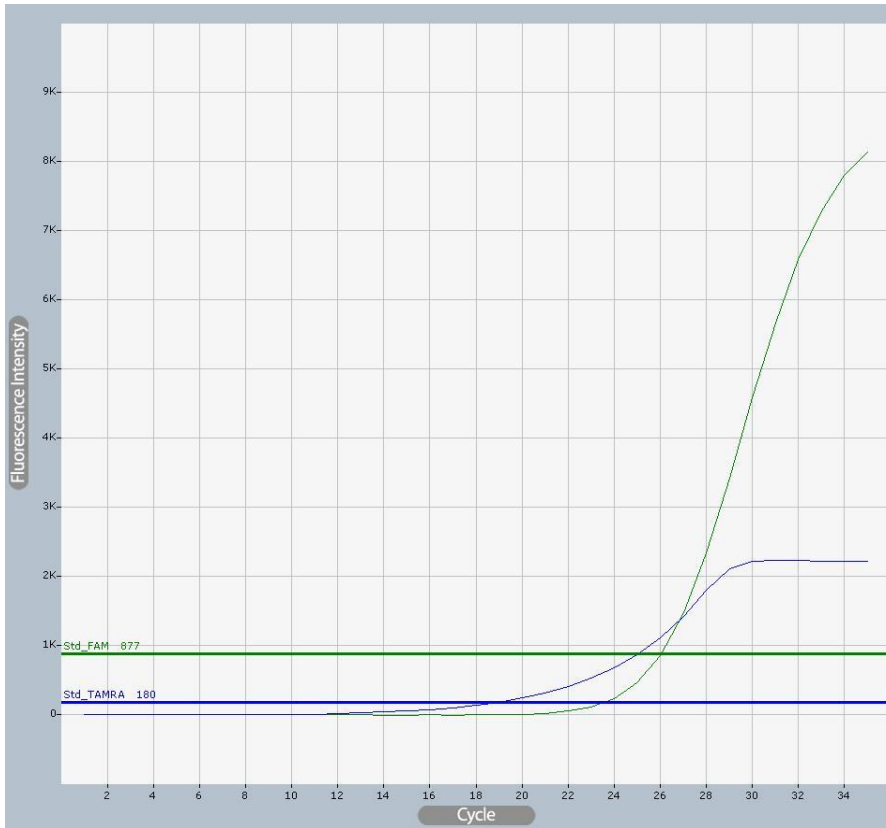

SNo.	Colour	Name	Type	Ct	Given Conc (copies)	Calc Conc (copies)
1	■	ATINDER 10208002-6230	HLA B-27	26.04	NA	NA
2	■	ATINDER 10208002-6230	IPC	18.87	NA	NA