


## QUANTIFICATION REPORT

### Experiment Information:

Assay Type	HBV DNA Absolute Quantification
User	IMMUNO DIAGNOSTICS PVT. LTD.
Instrument S/N	Bio-Rad CFX96™ REAL-TIME System
Run Date	10/23/2023 15:12PM

### QUANTIFICATION DATA FOR SAMPLE: SURENDER-39481

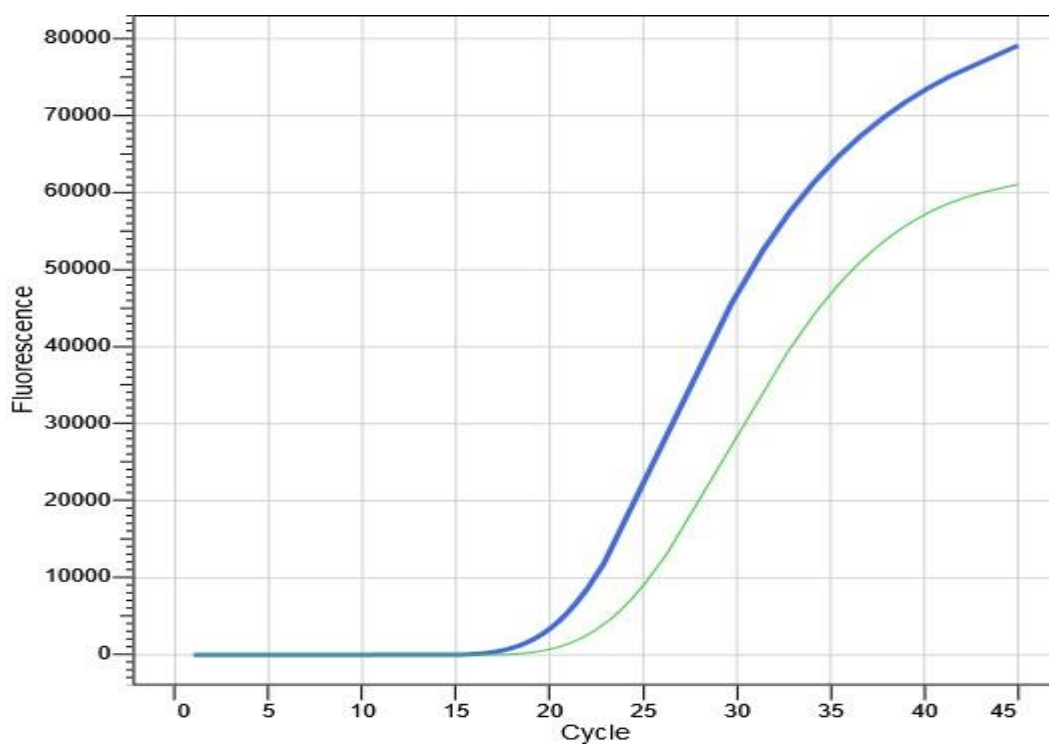

S. No.	Colour	Name	Type	Ct	Given Conc. (copies)	Calc. Conc.
1	■	SURENDER-39481	HBV	20.55	NA	43800000.7 IU/mL
2	■	SURENDER-39481	IPC	24.11	NA	NA

This report is generated by Bio-Rad™ CFX Manager IVD Edition 1.6 (Admin.)